

# Pipe Crawler<sup>®</sup> Internal Piping Characterization System

Deactivation and  
Decommissioning Focus Area



*Prepared for*  
**U.S. Department of Energy**  
Office of Environmental Management  
Office of Science and Technology

February 1998

---

## **DISCLAIMER**

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

# Pipe Crawler<sup>®</sup> Internal Piping Characterization System

OST Reference # 1810

Deactivation and  
Decommissioning Focus Area



*Demonstrated at*  
Chicago Pile 5 (CP-5) Research Reactor  
Large-Scale Demonstration Project  
Argonne National Laboratory-East  
Argonne, Illinois

# **INNOVATIVE TECHNOLOGY**

*Summary Report*

## ***Purpose of this document***

Innovative Technology Summary Reports are designed to provide potential users with the information they need to quickly determine if a technology would apply to a particular environmental management problem. They are also designed for readers who may recommend that a technology be considered by prospective users.

Each report describes a technology, system, or process that has been developed and tested with funding from DOE's Office of Science and Technology (OST). A report presents the full range of problems that a technology, system, or process will address and its advantages to the DOE cleanup in terms of system performance, cost, and cleanup effectiveness. Most reports include comparisons to baseline technologies as well as other competing technologies. Information about commercial availability and technology readiness for implementation is also included. Innovative Technology Summary Reports are intended to provide summary information. References for more detailed information are provided in an appendix.

Efforts have been made to provide key data describing the performance, cost, and regulatory acceptance of the technology. If this information was not available at the time of publication, the omission is noted.

All published Innovative Technology Summary Reports are available online at <http://em-50.em.doe.gov>.

---

## SECTION 1

# SUMMARY

### Technology Summary

---

#### Problem

Radiologically contaminated piping systems are a major problem in U.S. Department of Energy (DOE) and commercial facilities planned for decontamination and decommissioning (D&D). Performing radiological surveys of pipes provides information on type and degree of contamination to facilitate decisions regarding disposition of piping systems. For example, accurate data can support decisions to reuse pipes or to economically decontaminate pipes, therefore gaining free release of intact piping systems and, thus, avoiding the disposition of all pipes as low-level. The Pipe Crawler<sup>®</sup> technology, used as part of a complete pipe management program, offers a number of distinct advantages over a baseline approach to excavate and dispose of piping as low-level waste.

#### How it Works

Pipe Crawler<sup>®</sup> is a pipe surveying system for performing radiological characterization and/or free release surveys of piping systems. The technology employs a family of manually advanced, wheeled platforms, or crawlers, fitted with one or more arrays of thin Geiger Mueller (GM) detectors operated from an external power supply and data processing unit. Survey readings are taken in a step-wise fashion. A video camera and tape recording system are used for video surveys of pipe interiors prior to and during radiological surveys. The 12-in-diameter crawler used in the demonstration is shown in Figure 1.

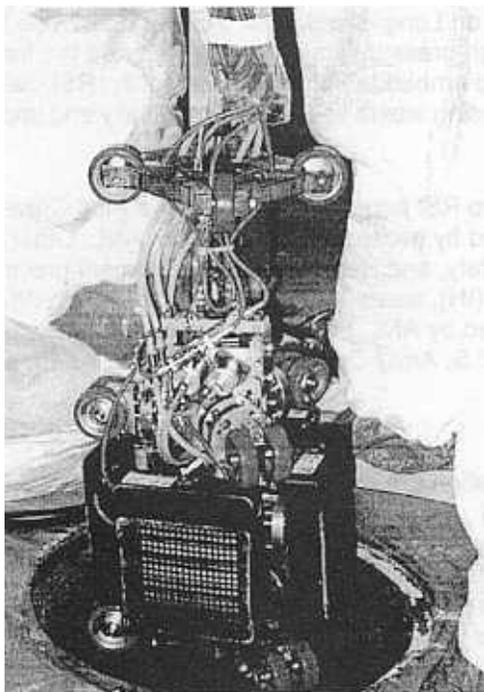


Figure 1. Pipe Crawler<sup>®</sup>-12-in model-being lowered into below-grade storage hole.

#### Advantages Over the Baseline

Pipe Crawler<sup>®</sup> has potential advantages over the baseline and other technologies in areas of cost, durability, waste minimization, and intrusiveness. Advantages include potentially reduced cost, potential reuse of the pipe system, reduced waste volume, and the ability to manage pipes in place with minimal disturbance to facility operations. Advantages over competing technologies include potentially reduced costs and the ability to perform beta-gamma surveys that are capable of passing regulatory scrutiny for free release of piping systems.



## Commercial Availability

The technology is currently offered as part of a turnkey service provided by Radiological Services, Inc.'s (RSI) Pipe Crawler<sup>®</sup> technology to inspect, decontaminate, and survey piping systems for free release. Individual crawlers for pipes with diameters ranging from 2–18 in have been built employing commercially available detectors and analyzers in custom-made arrays and crawlers. The units are manually advanced through pipes using flexible fiber glass rods attached to either end. Pipe lengths up to 200 ft in length containing multiple 90° bends can be surveyed in this manner.

## Demonstration Summary

---

This report presents an evaluation of RSI's Pipe Crawler<sup>®</sup> technology for performing radiological surveys of piping systems. The evaluation is based largely on the performance of the system as part of the Large-Scale Demonstration Project (LSDP) held at the Chicago Pile-5 (CP-5) Research Reactor located at Argonne National Laboratory-East (ANL-E). The LSDP is sponsored by DOE's Office of Science and Technology, Deactivation and Decommissioning Focus Area (DDFA). The objective of the LSDP is to demonstrate innovative technologies or technology applications potentially beneficial to the decontamination and decommissioning of contaminated facilities.

The Pipe Crawler<sup>®</sup> technology application data collected from the demonstration at CP-5 should be broadly applicable to many D&D projects. CP-5 is a heavy-water moderated and cooled, highly-enriched, uranium-fueled thermal reactor designed to supply neutrons for research. The reactor had a thermal-power rating of 5 megawatts and was continuously operated for 25 years until its final shutdown in 1979. Such operation has produced D&D characteristics representative of other nuclear facilities within the DOE Complex and in other research and commercial reactors.

Prior to use at CP-5, the major application of the technology was during the decommissioning of the Shoreham Nuclear Power Plant on Long Island, New York in 1992. Pipe Crawler<sup>®</sup> surveys performed after decontamination of piping by high-pressure water wash supported the free-release approval of over 15,000 linear ft of drain lines and embedded piping at the facility. RSI claimed to have saved over \$10 million on that project while reducing waste volumes dramatically and improving worker safety when compared to demolition.

For the LSDP demonstration, two RSI personnel operated the Pipe Crawler<sup>®</sup> system and recorded the survey data while being observed by two test engineers from ANL. Other ANL personnel from the CP-5 facility and the Environment, Safety, and Health (ESH) Department provided support in the areas of health physics (HP), industrial hygiene (IH), waste management operations (WMO), and safety engineering. Demonstration data was collected by ANL, and data for cost analysis was provided by ANL and RSI. Cost analysis was performed by the U.S. Army Corps of Engineers USACE), and benchmarking activities were performed by ICF Kaiser.

### Key Results

The key results of the demonstration are as follows:

- Pipe Crawler<sup>®</sup> successfully demonstrated its ability to perform characterization of radioactive contamination in buried and embedded piping. This offers the potential for significant cost savings over the baseline approach to excavate, dismantle, and dispose of piping. For the CP-5 project, this cost savings (based on the demonstration results vs. anticipated costs based on the CP-5 cost estimate) was approximately \$27,934 or 45 percent of the original cost estimate. However, this value is specific to the CP-5 facility; a cost comparison must be based on facility-specific criteria for other sites.

Based on the observed performance of the technology in piping systems and after evaluation of calibration and quality assurance procedures, it appears that the technology is capable of making activity measurements inside piping systems that are of sufficient quality to support free-release decisions.

Radiological surveys were performed in 13 rod storage holes of 5 in, 6 in and 12 in diameter and with a total length of 162 ft and in 25 ft of two 12-in-diameter embedded vent lines.



At least 30 percent of the interior surfaces of pipes was measured by the detector arrays by advancing the various crawlers in appropriate increments.

Counting times of one min at each increment gave sufficient detectability for characterizing contamination near background and ample detectability near the release limit.

Activity levels in rod storage holes ranged from background levels to greater than 190 times the release limit; levels in the vent lines were at or near background.

Surveys in rod storage holes with highest activity levels did not cause significant equipment contamination nor cross-contamination of subsequent holes.

The equipment functioned at regular throughput rates in the tested lines with only minor problems or delays, the most significant being a broken detector from debris in a line.

Calibration of the detector arrays, using a calibration source with activity uniformly distributed at the action level in a plastic sheet used to line a calibration pipe, inspires confidence in the survey readings, particularly near the 5000 disintegrations per minute (dpm)/100 cm<sup>2</sup> action level.

The use of the flexible fiber glass rods proved to be an effective means of advancing the crawlers and for confidently metering stepwise movements.

Operation of the technology required the full attention of two technicians; prolonged use of the equipment could be physically taxing.

---

## Contacts

### Technical

Jim McCleer, Radiological Services, Inc., New London, Connecticut, (860)-443-4944

### Demonstration

Kurt Picel, Test Engineer, Argonne National Laboratory, (630) 252-4018, kcpicel@anl.gov

Charles Roche, Test Engineer, Argonne National Laboratory, (630) 252-3432, ctroche@anl.gov

### CP-5 Large-Scale Demonstration Project or Strategic Alliance for Environmental Restoration

Richard C. Baker, U.S. Department of Energy, Chicago Operations Office, (630) 252-2647, richard.baker@ch.doe.gov

Steve Bossart, Federal Energy Technology Center, (304) 285-4643, sbossa@fetec.doe.gov

Terry Bradley, Strategic Alliance Administrator, Duke Engineering and Services, (704) 382-2766, tlbradle@duke-energy.com

### Licensing Information

No licensing or permitting activities were required to support this demonstration.

### Web Site

The CP-5 LSDP Internet address is <http://www.strategic-alliance.org>.

### Other

All published Innovative Technology Summary Reports are available online at <http://em-50.em.doe.gov>. The Technology Management System, also available through the EM50 Web site, provides information about OST programs, technologies, and problems. The OST Reference # for Pipe Crawler® is 1810.



## SECTION 2

# TECHNOLOGY DESCRIPTION

### Overall Process Definition

---

Pipe Crawler<sup>®</sup> is a manually deployed pipe inspection system that consists of a platform, or crawler, mounted with a 360° array of thin Geiger Mueller (GM) tubes for detection of activity, connected by cable to an external data processing and storage system. A family of crawlers is used to accommodate various piping sizes. The dimensions of a given crawler must be close to the size of pipe to be surveyed. This ensures that the precise geometry and close mating of detectors to interior pipe surfaces can be maintained, which is afforded by a spring-loaded wheel suspension system. Each crawler is custom made, employing commercially available thin membrane GM tubes. The size and shape of the available GM tubes strongly influences the configuration and overall design of a given crawler. The smaller crawlers for pipes with diameters less than 8 in are manually deployed using flexible fiberglass rods attached to either end. The rods are similar to those used by plumbers. The larger crawlers for 8-in-diameter and larger pipes employ pneumatically-operated positioning systems.

Pipe crawlers are generally deployed in a manner that results in less than complete coverage of pipe interior surfaces. At Shoreham, a uniform coverage of 30 percent or more was sufficient to establish the contamination status of piping to the satisfaction of the Nuclear Regulatory Commission (NRC). The desired level of coverage is achieved through a combination of number, size and geometry of the GM detectors and the size of the advancement steps used in surveys. Crawlers for pipes under 8 in diameter typically employ two detector arrays of three detectors each. The two offset arrays of the 6-in crawler can be seen in the photograph in Figure 1. The two arrays are rotationally offset from one another to maximize coverage along the circumference of pipes, while they are set at a fixed distance from each other along the length of pipe. This separation distance is factored in with the desired coverage rate to calculate the size of step increments.

Crawlers for 8-in and larger pipes use only a single detector array containing typically four GM detectors. Multiple fixed arrays would be too bulky to maneuver easily through piping. These crawlers employ compressed air to extend and retract the detector array to ease movement and to rotate the detector array at each step location. The latter movement has the effect of having a second array mounted in an offset position, as in the smaller crawlers. A small, 40 ft<sup>3</sup>/min, 100 psi air compressor is used to operate the pneumatic system.

A schematic diagram of the complete, integrated, Pipe Crawler<sup>®</sup>/video recording system is shown in Figure 2. The video system is assembled mainly from commercially available components, including a compact video camera. Custom-made parts needed to complete the pipe inspection system include a wheeled camera mount, or "dogbone," and a microprocessor chip allowing communication of the commercially available Eberline ESP-2 data processing module holding radiological survey data with the VHS videotape recording system. This modification of the ESP-2 allows survey readings from various crawlers to be recorded directly on videotape so that visual features within piping can be associated with survey readings taken at the same location.

### System Operation

---

#### GM Detector Arrays

The Pipe Crawler<sup>®</sup> employs arrays of three or four thin profile, or "pancake," GM detectors. These commercially available detectors employ an ionizing gas encased in a plastic membrane. They typically operate under an applied bias of 900 V. Efficiencies vary with type and energy of the incident radiation. For cobalt-60, the isotope generally used for calibration, efficiencies range from around 7 percent to around 14 percent for the detectors used in the 12-in and 6-in crawlers, respectively. In practical applications, the detector surface must be held in close proximity, i.e., within 1 cm of the measured surface, for reliable detection of alphas, which have a limited range in air.



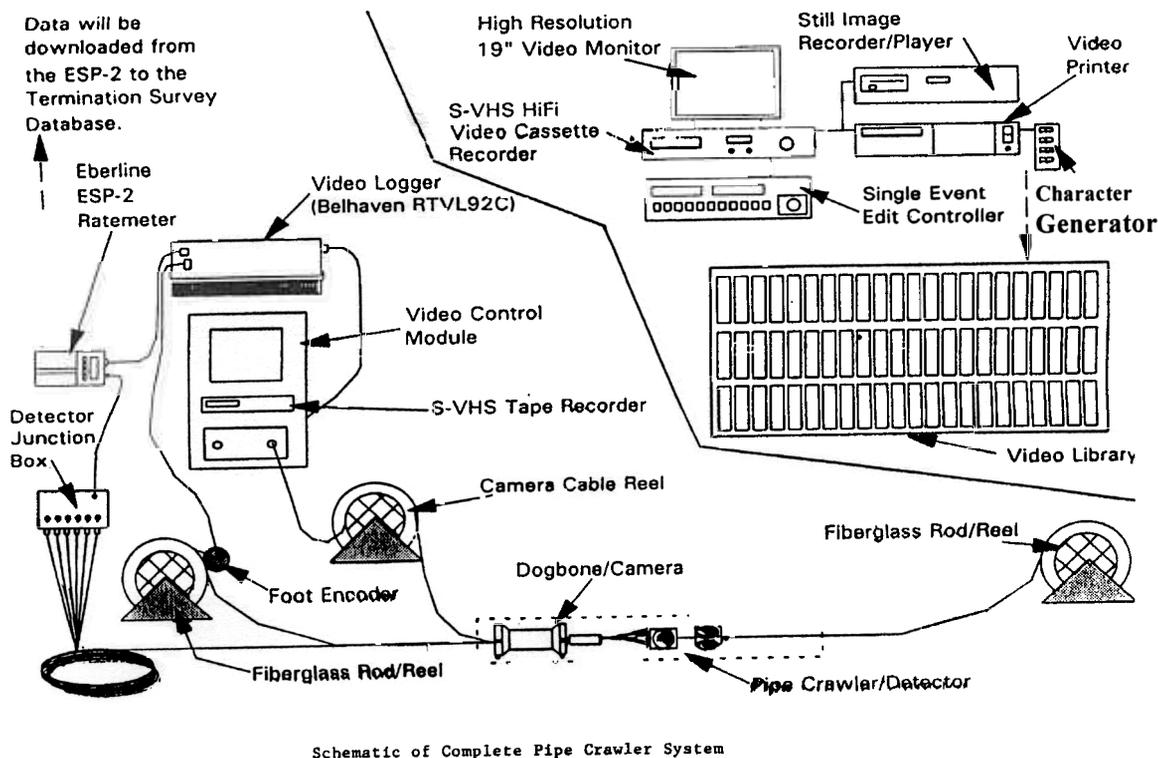


Figure 2. Schematic of complete Pipe Crawler<sup>®</sup> system.

### Calibration of Detector Arrays

Detector arrays are calibrated to a radiation source of known strength so that the relationship between detector count rate and source strength can be determined. To this end, detector efficiency for Pipe Crawler<sup>®</sup> arrays is determined directly using a "standard pipe," rather than using point sources and accounting for detector geometry. The former method is more direct, faster, simpler, and more repeatable than the latter. It employs special calibration sources that are uniformly dispersed within mylar sheets. The activity of the calibration sources are near the 5000 dpm/100 cm<sup>2</sup> action level.

A crawler of a given size is placed in a matching plastic calibration pipe that is lined with the sheet source. The detector array count rate for the known activity per unit area is then determined. The total viewing area of all the detectors in the array is then factored to determine efficiency in terms of counts per min per dpm/100 cm<sup>2</sup>, after background from the calibration pipe without the source is subtracted.

Several different sizes of Pipe Crawler<sup>®</sup> have been built for pipes from 2 in–18 in internal diameter. Two units were demonstrated at CP-5, a 6-in and a 12-in unit. The 6-in unit was modified by removing its wheels to accommodate the 5-in rod storage holes. The 12-in unit was used in both the 12-in rod storage holes and in the 12-in cast iron vent line.

### Other Conditions and Considerations

- Pipe Crawler<sup>®</sup> is lightweight (less than 50 lb), portable (18 in by 36 in), and can be maneuvered by hand.
- The utilities required for the unit include a source of 40 ft<sup>3</sup>/min, 100 psi air pressure and a 115 V, 20 amp electrical current source.
- Pipe Crawler<sup>®</sup> cannot differentiate specific isotopes or radiation types.



- Pipe Crawler® cannot be used in pipes containing or suspected of containing standing water because of the high voltage used in the detectors.
- A moderate level of skill and training is required to operate the equipment.

No secondary waste streams, beyond disposable personal protective equipment (PPE) for operators and rags for wiping down equipment, were generated by the radiological surveys.



## SECTION 3

# PERFORMANCE

### Demonstration Plan

---

The demonstration of RSI's Pipe Crawler<sup>®</sup> technology was conducted according to the approved test plan *CP-5 Large-Scale Demonstration Project: Test Plan for the Demonstration of the Pipe Crawler System at CP-5*. The performance of the Pipe Crawler<sup>®</sup> technology was evaluated against the baseline technology—excavation and disposal. The principal objective of the demonstration was to establish that the Pipe Crawler<sup>®</sup> technology could perform radiological surveys of piping systems to allow the systems to be released without restrictions or reused for clean application. Of particular interest were embedded piping systems that would be very costly to manage by excavation and disposal as low-level waste.

Several embedded piping systems in CP-5 were identified as candidates for surveys through discussions with facility personnel and review of available drawings. The identified piping systems included pipes with internal diameters from 3 in–18 in, both horizontal and vertical in configuration, ranging in length from 10 ft–150 ft, and constructed of a variety of materials. Specific piping systems included a 4-in (3-in-internal diameter) by 150-ft drain line of vitreous clay, two 12-in by roughly 150-ft cast iron air vent lines, and an array of fuel rod storage holes from 10 ft–17 ft in depth. The latter holes had diameters of 5 in, 6 in, or 12 in, arranged vertically in a block of concrete sunk into the floor of the Rod Storage Area and lined with either stainless steel or carbon steel.

The 4-in drain line was eliminated from consideration when it was learned that it had a high probability of containing standing water, a condition incompatible with the high voltage used in the GM detectors. Similarly, a decision was made to not perform surveys in the 12-in vent lines beyond 90° bends roughly 20 ft in from the point of access to ensure that the crawler could be extracted from the line. The crawler could only be manipulated from one end in these lines, and video inspection further revealed mismatched pipe joints, presenting potential snag points. To compensate for these reductions in scope, the number of planned rod storage holes to be surveyed was increased from 6 to 13.

### Treatment Performance

---

Pipe Crawler<sup>®</sup> successfully demonstrated its ability to characterize radioactive contamination above background levels in buried and embedded pipes.

Pipe Crawler<sup>®</sup> demonstrated its ability to produce repeatable characterization results.

Use of the Pipe Crawler<sup>®</sup> manual deployment equipment (i.e., flexible fiberglass rods) required some physical exertion on the part of personnel to advance the crawler and cables.

Pipe Crawler<sup>®</sup> was easy to wipe down between uses to remove contamination. Although the potential existed for contamination to be entrained with Pipe Crawler<sup>®</sup> as it was removed from one pipe and inserted into another, cross-contamination of pipes did not occur.

Use of Pipe Crawler<sup>®</sup> did not result in the generation of secondary waste other than personal protective clothing and rags used to wipe down the equipment.

Survey results from the demonstration are summarized in Table 1. The results indicate a general picture of the level of activity in each hole or line surveyed that can be compared to release criteria (i.e., generally 5000 dpm/100 cm<sup>2</sup>) to gain an indication of what actions might be appropriate or required to close out the management of the rod storage holes and 12-in vent line.



## Rod Storage Holes (RSH)

As indicated in Table 1, surveys were performed on 13 rod storage holes, composed of five 5-in, four 6-in, and four 12-in holes. The surveys were made with two different crawlers. The first was used for the 5-in and 6-in holes; and the second was used for the 12-in holes. The standard step sizes used were 4 in and 12 in, respectively, for the first and second crawlers, resulting in coverages exceeding 30 percent, the presumed standard for regulatory acceptance. Nonstandard step sizes were used for more rapid surveys of additional holes, after at least two holes of each size were surveyed with the standard step sizes. For example, hole #52 was known to be highly contaminated so only four readings were taken with the 6-in crawler at 24-in intervals to get a simple profile of the hole.

Similarly, a standard count time of one min was used to ensure sufficient counting statistics at low activities. Occasionally, in the interest of time, a 30-s count time was used. The shorter count time gave a sufficient number of counts, even at low activities, for confident results. With the 1-min count times and standard step sizes, the 10-ft-depth, 5-in holes required about 40 min to survey, while the 14-ft-depth, 6-in and 12-in holes required about 1 h each, including time to remove and replace plugs and wiping down cables and equipment after each survey.

Survey readings in counts per min (cpm) for all surveys were stored in the ESP-2 data processing unit. These readings were manually converted to dpm/100 cm<sup>2</sup> by RSI after the demonstration using an appropriate calibration algorithm. The latter results were tabulated and manually plotted as a profile for each hole or line surveyed for comparison to the 5000 dpm/100 cm<sup>2</sup> release standard. Figure 3 is an example profile for 6-in rod storage hole #42, which was surveyed in triplicate to evaluate the reproducibility of surveys.

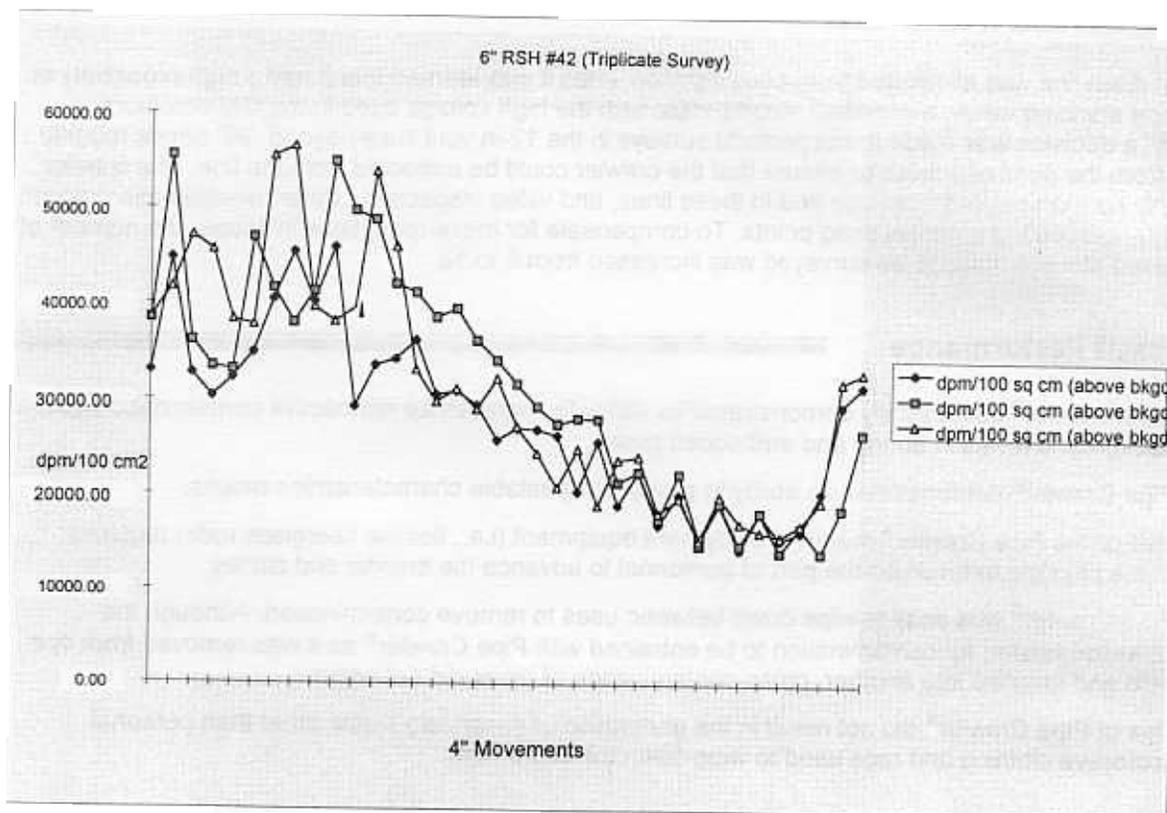


Figure 3. Example contamination profile for rod storage hole #42

The activity levels measured in the various holes varied widely, as shown in the two right-hand columns of Table 1. The background levels in the 5-in and 6-in holes were determined to be 272 cpm and 639 cpm beta-gamma, respectively, measured by the various detector arrays. Within a single hole, activities could vary from background levels to over 50 times the release standard of 5000 dpm/100 cm<sup>2</sup>. Holes #4 and #39 had no readings above the release limit, while holes #8, #43, and #68 had some readings just over the limit. The remaining holes generally had levels well over the limit. All three size groups had at least one



relatively uncontaminated hole and one or more highly contaminated holes. While the 5-in holes were lined with stainless steel and had a much smoother finish than the corroded carbon-steel-lined 6-in and 12-in holes, the three sets of holes exhibited similar ranges of activity. This result suggests little apparent effect on activity levels from the type of steel nor its appearance, assuming similar use patterns.

Survey results for the various rod storage holes could support decisions with respect to the holes. The activity levels observed in many of the holes indicate a need for substantial decontamination if they are to be left in place, while other holes would require little or no decontamination for release. These results could be used to identify the type and extent of decontamination that would be required to address the surveyed holes. Moreover, to the extent the 13 surveyed holes represent the entire 76-hole array, costs could be estimated to decontaminate and release the entire array.

**Table 1. Summary of Pipe Crawler<sup>®</sup> survey results for the CP-5 rod storage holes and portions of the 12-in vent lines**

Hole or Vent No.	Inside diameter (in)	Depth or Length (ft)	Step Size (in)	# Survey Readings	Approx. Coverage (percent)	Count Time (min)	Activity Range Total $\beta/\gamma$ (dpm/100cm <sup>2</sup> )		Activity Mean Total $\beta/\gamma$ (dpm/100cm <sup>2</sup> )
							min	max	
4	5	10	8	14	20	0.5	0	998	270
8	5	10	8	14	20	0.5	798	7805	1,986
	5	10	4	25	37	1.0	919	399,367	
	5	10	4	24	37	1.0	28,407	343,161	
	5	10	4	25	37	1.0	8,394	37,390	
	6	14	8	17	18	1.0	0	3,051	
42 (1)	6	14	4	36	37	1.0	14,398	45,442	28,242
42 (2)	6	14	4	36	37	1.0	14,188	54,950	31,612
42 (3)	6	14	4	36	37	1.0	15,343	56,526	31,212
43	6	14	4	36	37	1.0	2,526	8,094	4,953
52	6	14	24	4	4	1.0	145,825	248,782	189,556
61	12	14	12	30	36	0.5	11,767	952,159	193,830
65	12	14	12	32	36	1.0	2,070	13,152	3,868
68	12	14	12/6	26	30	1.0/0.5	0	8,250	
71	12	14	12	32	36	1.0	0	228,552	30,197
VL1-F	12	21	12	42	36	0.5	0	943	242
VL1-R	12	21	12	42	36	1.0	(-64)	508	216
VL2-F	12	4	8	8	40	1.0	223	411	302

A cost analysis of the Pipe Crawler<sup>®</sup> technology developed from the demonstration is presented in Section 5. Costs to characterize piping are compared to the baseline approach of pipe dismantlement and disposal. In the case of the rod storage holes, dismantlement would involve removing and size reducing the steel liners and coring out the unlined hole. The removed material would then be disposed as low-level waste. In this case, the savings accrued by Pipe Crawler<sup>®</sup> surveys could be considered costs avoided for unnecessarily dismantling any holes in this manner that were established by survey to be suitable for free release. Further savings could be estimated for holes requiring only simple decontamination rather than dismantlement and coring.

Another consideration in favor of employing a decontaminate-and-survey approach here is that the rod storage holes are straight vertical holes with no joints, fittings, or obstructions. This makes the holes easy to survey and decontaminate if necessary. Also, such an approach would be far less disruptive to CP-5 activities and would pose lower overall risks to D&D workers and facility personnel.



## 12-in Vent Lines

The 12-in vent lines were a pair of cast iron air lines that serviced the reactor area. The lines were accessible from a shallow well in the vestibule area of the main floor outside the central containment area of CP-5. The lines run under the concrete floor of the facility, exiting to the northeast and making a 90° bend to the right at a point roughly 20 ft from the access point. The lines then run underground roughly 130 ft to the location of the former ventilation annex where the lines are currently capped and buried.

Surveys of the 12-in vent lines were performed with the same 12-in crawler using the same methodology as used in the 12-in rod storage holes. The results of the Pipe Crawler® surveys for the 12-in vent lines are shown at the bottom of Table 1. The left-hand line (when facing the openings) was surveyed at 12-in steps with two readings at offset positions at each step. Readings were taken in the forward (VL1-F) and reverse (VL1-R) directions producing a duplicate survey of the initial portion of the line. Near the end of the reverse survey, one of the four detectors was pierced by a piece of debris. Readings over the last five ft of the reverse survey (near the access point) had to be corrected for the broken detector.

Time constraints limited the survey of the second line (VL2-F) to four steps at 8-in intervals using 1-min count times to adjust for the broken detector. These readings provided a nominal measure of activity levels at the mouth of the second line.

Readings in the first line ranged only as high as twice background near the mouth, falling to background within a few ft. The few readings in the second line were near background. All readings for both lines were below levels requiring decontamination in the surveyed portions near the line starting point in CP-5. There is no apparent reason to expect levels to rise again in the remaining portions of the lines buried outside the facility. This conclusion is stronger for the first line than the second line where only a few measurements were made. These survey results in conjunction with a review of the process history of the two lines support at least a preliminary conclusion that the two 12-in vent lines require no remedial action.

The application of the Pipe Crawler® technology in the vent lines exemplifies the kind of savings that might be accrued with the technology under the best circumstances. The demonstration surveys of the lines required only a few hours of work with a two-person crew and produced quality results that could support a decision that no further action was necessary. The demonstration performance suggests that substantial portions of the two lines could be surveyed in a day or two with sufficient quality to support release of the lines. The cost of such surveys would compare very favorably to presumptive excavation and disposal of the two embedded 150-ft lines.



## SECTION 4

# TECHNOLOGY APPLICABILITY AND ALTERNATIVES

### Competing Technologies

---

The baseline technology approach that competes with the Pipe Crawler<sup>®</sup> is excavation and disposal of embedded piping. This approach may require extensive time and equipment to complete and may be potentially unnecessary if the pipe is uncontaminated.

Competing technologies include the following:

- Pipe Explorer<sup>™</sup>, developed by Science and Engineering Associates, Inc. Also demonstrated as part of the CP-5 LSDP, Pipe Explorer<sup>™</sup> is a pipe characterization system that employs an air-tight membrane deployed from a canister with air pressure to line the interiors of pipes and to carry a tether to which detectors are attached. As the membrane deploys, detectors are towed along inside the membrane while measurement data is collected.
- Multisensor Inspection and Characterization Robot for Small Pipes (MICROSPI) developed by Lockheed Martin Astronautics
- Internal Duct Characterization System developed jointly by Idaho National Engineering and Environmental Laboratory, Inuktun Services, Ltd., and Automation Systems Associated, Ltd. (the latter two located in British Columbia)
- Small Pipe Characterization System (SPCS) developed by Foster-Miller, Inc.

A comparison of the relative characteristics, benefits, and limitations of these technologies will be provided in the LSDP final report.

Advantages of the Pipe Crawler<sup>®</sup> technology include the following:

- Pipe Crawler<sup>®</sup> covers a wide range of pipe sizes, lengths and materials.
- Surface coverage can be adjusted to any desired level to meet release requirements.
- Detector arrays have ample sensitivity relative to release limits.  
Detector array calibration is straightforward using the dispersed calibration sources.
- Maintenance of precise detector geometry during surveys assures accurate readings.
- Calibration control charts, daily response checks, and detector array “knockdowns” lend further confidence to the reliability of measurements.
- Use of off-the-shelf detectors and other components simplifies repairs and increases up time.  
The system generates little or no waste.

Limitations of the Pipe Crawler<sup>®</sup> technology include the following:

Different-sized units are required for nominally different pipe sizes.

Cannot be used in pipes with standing water.

Pipes must be free of obstructions or accessible from either end of an obstruction.



Crawlers can become contaminated if used in untreated pipes. (However, only minor contamination of low-cost wheels occurred during the demonstration from loose corrosion in the untreated pipes.)

Pipes accessible from only one end present difficulties in manipulating and recovering crawlers.

Technology is not particularly suited to detection of alpha contamination.

Video inspection revealed mismatched pipe joints presenting potential snag points.

## Technology Applicability

---

The Pipe Crawler® technology is applicable to a wide range of pipe sizes and materials. Units have been built for pipes ranging in internal diameter from 2 in–18 in. Most pipe materials can be surveyed, including steel, stainless steel, cast iron, and vitreous clay. The most important factors affecting the suitability of pipe systems are smoothness, types of joints, number and sharpness of bends, and freedom from obstructions and debris. Pipe lengths up to 200 ft can be surveyed if accessible from both ends. Single-end access reduces the range to about half and makes manipulation and recovery of the units more difficult. Drain pipes are particularly suited to the technology as they are typically fairly straight and uncomplicated systems and are often embedded, which increases the benefit of in-place management.

## Patents/Commercialization/Sponsor

---

No issues related to patents, commercialization, or sponsorship are pending. Pipe Crawler® is a commercially available technology.



## SECTION 5

# COST

### Introduction

---

This cost analysis compares the relative costs of the innovative and baseline technologies and presents information that will assist D&D planners in decisions about use of the innovative technology in future D&D work. This analysis strives to develop realistic estimates that represent D&D work within the DOE Complex. However, this is a limited representation of actual cost because the analysis uses only data observed during the demonstration. Some of the observed costs will include refinements to make the estimates more realistic, such as elimination of cost factors only applicable to demonstration of technologies. These are allowed only when they will not distort the fundamental elements of the observed data (e.g., do not change the productivity rate, quantities, and work elements, etc.) and eliminates only those activities which are atypical of normal D&D work. The *CP-5 Large-Scale Demonstration Project, Summary of Results of Pipe Crawler Surveys for DOE's LSDP at CP-5* provides additional cost information.

### Methodology

---

This cost analysis for the Pipe Crawler<sup>®</sup> innovative technology is based upon data collected during the demonstration that includes duration of activities, work crew composition, equipment used in the performance of the work, and supplies used. Data was collected into a predetermined structure to foster consistency with other demonstrations. Following collection of the data, team members from ICF Kaiser, USACE, and a D&D technical specialist from the Argonne National Laboratory reviewed the costs and agreed on the approach used in the analysis. Those activities and costs that are for performance benchmarking (not a normal part D&D work) or that result from the demonstration nature of the contract are not included in this analysis.

The baseline technology was assumed to be dismantlement and removal of the contaminated pipes, and the cost estimate for that baseline is based upon a number of budget documents for the CP-5 including

- *Decommissioning Cost Estimate for Placing the CP-5 Reactor Facility into Safe Storage (SAFSTOR)*;  
*Decommissioning Cost Estimate for Full Decommissioning of the CP-5 Reactor Facility*, prepared for Argonne National Laboratory; and  
1996 activity cost estimates for the CP-5 decommissioning.

Since the baseline cost estimate is not based on observed data, extra effort is applied in setting up the cost analysis to assure unbiased and appropriate production rates and crew costs. Specifically, the previously mentioned team reviewed the activities and assumptions to be used in the baseline estimate to ensure a fair comparison with the Pipe Crawler<sup>®</sup> demonstration.

The cost estimates for both the baseline and the innovative technology follow the *Hazardous, Toxic and Radioactive Waste Remedial Action Work Breakdown Structure and Data Dictionary* (USACE, 1996) for collecting costs into cost elements for reporting. For those cost elements associated with equipment that is assumed to be purchased by ANL or is owned by a vendor providing service to ANL, the hourly equipment rates that are used in this cost analysis include maintenance costs (if any) and allow for depreciation and the facility's capital cost of money (FCCM) and is computed in accordance with the *Construction Equipment Ownership and Operating Expense Schedule* (USACE EP-1110-1-B, 1995). For those cost elements associated with equipment that is assumed to be rented, that rental rate is used. It is reasonable to assume that the rental rate includes consideration of repair costs, depreciation, and FCCM.



## Cost Analysis

The DOE Complex presents a wide range of D&D work conditions because of the variety of functions and facilities. The working conditions for an individual job directly affect the manner in which D&D work is performed and, as a result, the costs for an individual job are unique. The innovative and baseline technology estimates presented in this analysis are based upon a specific set of conditions or work practices found at CP-5 and are presented in Table 2. This table is intended to help the technology user identify work differences that can result in cost differences. The original baseline estimate for CP-5 assumed 165 linear feet (lin ft) of buried 6-in pipe would require remediation. Based on conditions found in the field, a total of 262 lin ft of various widths (5 in, 6 in and 12 in) was characterized using this technology. To ensure a fair and unbiased cost comparison, only 165 lin ft of the piping characterized was used for the comparative cost analysis. Since the costs were broken down to a per-linear-foot basis, and mobilization and demobilization costs for each respective technology are relatively fixed (see Figure 5 and Appendix C), this provided the most objective comparison of the two remediation methodologies.

**Table 2. Summary of cost variable conditions**

Cost variable	Pipe Crawler® technology	Baseline technology
<b>Scope of work</b>		
Quantity and Type of Material	74 ft of 5-in stainless steel pipe 72 ft of 6-in carbon steel pipe 116 ft of 12-in carbon steel & cast iron pipe (165 ft of pipe was used for price comparison purposes—see Appendix B)	165 ft of 6-in pipe
Location of test area	Rod storage and air lines for the reactor area	Reactor area
Nature of work	Only straight portions of pipe are surveyed and ends of 5-in and 6-in pipe are capped with a plug that requires a crane for removal.	Remove floor and excavate piping. Floor thickness of 1 ft. Assume only low-level radioactive contamination (no hazardous) so that there is not need to segregate sludge from pipe interior from the pipe (no need to try and reduce the volume of mixed waste).
<b>Work environment</b>		
Level of contamination in the test areas	Demonstration area is not a radiation area. Any contamination that might be present is fixed.	Respiratory protection not required for concrete removal. Area previously decontaminated. Pipe removal requires protective clothing and respirators.
Level of contamination inside the pipes	Two pipes below release limits. Five pipes near release limits. Remaining pipes were well above release limits.	Productivity loss factor for pipe removal portion of work assumed to be 2.02 which would include protective clothing and respiratory protection.
<b>Work performance</b>		
Acquisition means	Vendor provided service with mobilization of vendor equipment.	Local craft workers with rented equipment.
Compliance requirements	25 percent of pipe surface area is surveyed (assumes coverage that NRC historically accepted is adequate for site and regulators)	
Equipment & crew	Three crawler sizes and crew of two vendor personnel plus one HPT. (HPT support is a separate line item in the summary table.)	Backhoe loader, concrete saw, decontamination technician, operator and HPT.



**Table 2. Summary of cost variable conditions  
(continued)**

<b>Cost variable</b>	<b>Pipe Crawler® technology</b>	<b>Baseline technology</b>
Production rates	Crawler survey counts plus move to next increment is typically 1.2 min/increment with little variation based on timed observations. Video rate based on total time for video work divided by length of pipes.	Two ft <sup>3</sup> /h for concrete saw cut. Four ft <sup>3</sup> /h for concrete block removal. Seven ft <sup>3</sup> /h for pipe removal. Rates based on ANL budget documents.
Scale of production		
Process steps	<ol style="list-style-type: none"> <li>1. Remove pipe cap.</li> <li>2. Video pipe.</li> <li>3. Survey pipe.</li> <li>4. Performance check.</li> </ol>	<ol style="list-style-type: none"> <li>1. Saw cut concrete along pipe length.</li> <li>2. Cross cut into blocks.</li> <li>3. Remove concrete blocks.</li> <li>4. Cut pipe, and remove pipe and soil.</li> <li>5. Segregate contaminated soil. (This occurs as it is removed.)</li> <li>6. Dispose of waste.</li> </ol>
End condition	Pipe determined to meet free-release criteria remains in place. (Pipe not meeting release requirements will require further action.)	Pipe and concrete removed. (Open trench remains.)

The area is assumed to have been previously decontaminated, and this cost is not included in the baseline technology. However, the equipment used in the baseline technology must be decontaminated, and this cost is included in the estimate. The productivity loss factor accounts for inefficiencies associated with personal protective equipment (PPE), breaks, down time, etc.


## Cost Conclusions

For the conditions and assumptions of this demonstration, the innovative technology saves over 55 percent over the baseline alternative. A summary comparison is shown on Figure 4.


Figure 5 shows a comparison of the Pipe Crawler® to dismantlement per linear foot of pipe removed, based on the information and assumptions included in Appendix B. Fixed costs, including mobilization and demobilization, are assumed to be incurred regardless of the amount of pipe removed. Variable costs, including pipe characterization for the Pipe Crawler® and dismantlement and waste disposal for the baseline technology, are reduced to a dollar-per-foot value. This figure should be taken as a rough indication on when the innovative technology becomes cost effective. Actual crossover will be greatly influenced by site-specific parameters. Additionally, the Pipe Crawler® cost does not account for any pipe that may require dismantlement, based on the results of the Pipe Crawler® characterization.

The amount of savings realized by using the Pipe Crawler® technology will vary depending upon site-specific conditions and work requirements. The most prominent of these factors that influence the savings are the size of the job and the ability to free release the pipe following the Pipe Crawler® survey. In situations where a pipe is surveyed and fails the free-release requirements, decontamination of the pipe or dismantlement and disposal of the pipe will be required. Approximately \$13,000 of the Pipe Crawler® cost (65 percent of the total in this demonstration) is for mobilization and demobilization, and these costs remain relatively constant despite the number of pipes surveyed. Those facilities with larger pipe survey quantities will distribute the mobilization and demobilization over a larger job.



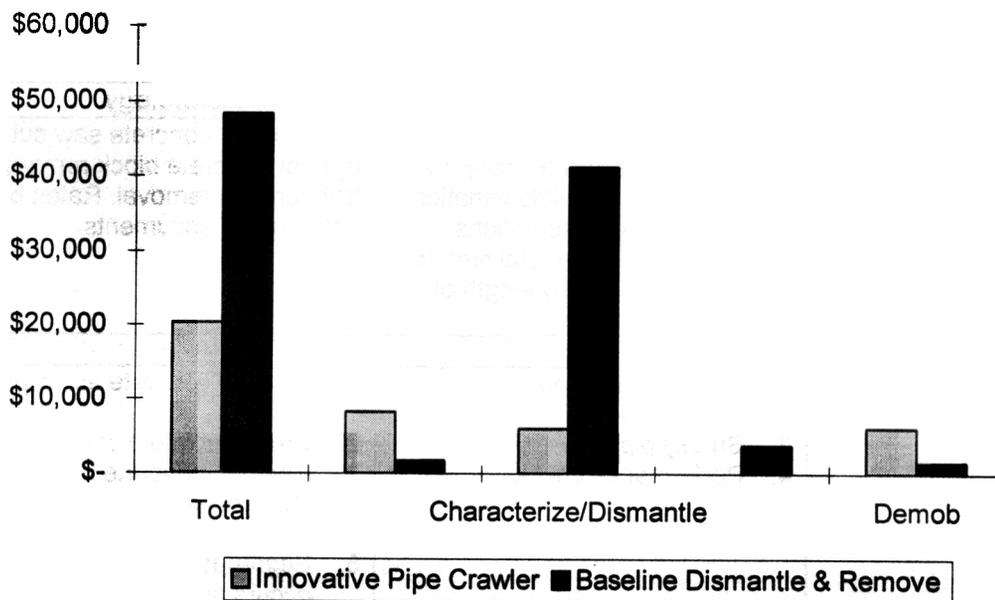

**Figure 4. Cost analysis summary comparison.**

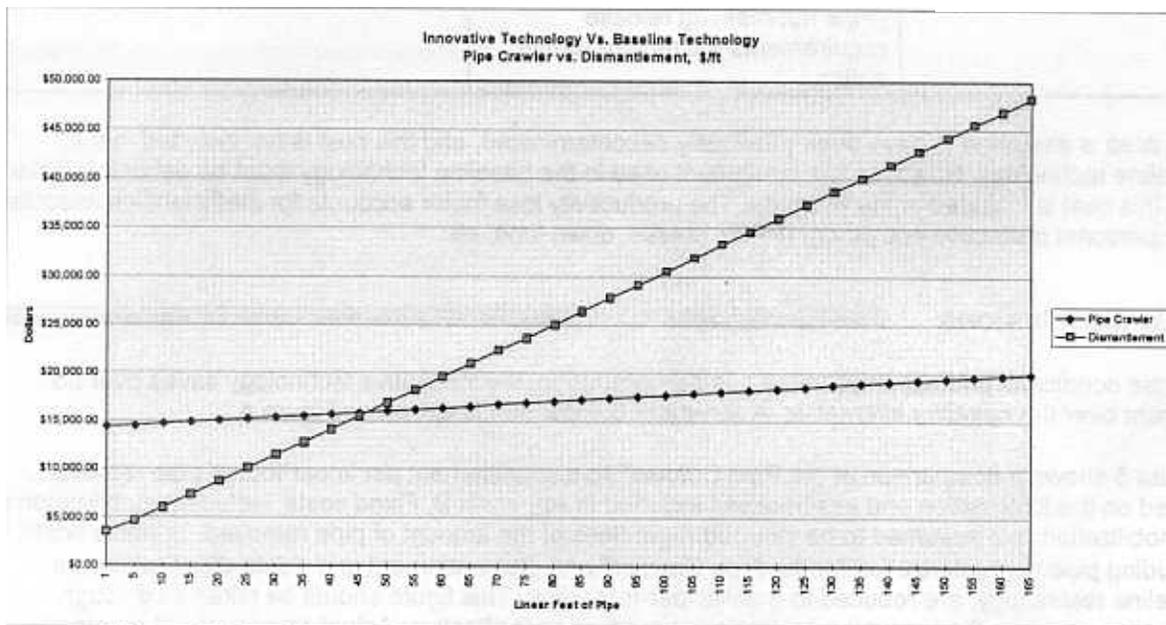

**Figure 5. Cost/linear foot comparison of innovative Vs. baseline technology.**

The total cost for the innovative technology is moderately sensitive to the mobilization and demobilization distance. Those sites located closer to the vendor will experience lower costs as compared with the more remote sites.

Establishing background radiation levels may be necessary where well documented survey results are required. The costs for establishing background is not included in this analysis, and that cost must be added for those situations. This will slightly reduce the potential savings but is not a large cost factor.

The baseline cost is sensitive to several parameters. Concrete slab thickness and width of the trench are significant cost drivers because changes in these dimensions result in changes to the concrete cutting production rate and waste disposal quantity. Additionally, the assumptions for the type of contamination are important factors in the total cost. If hazardous waste is present in addition to radioactive contamination, then efforts to scrape the sludge from the pipe interior may be required so that the pipe can be disposed as low-level radioactive waste rather than mixed waste. The waste assumptions in this



analysis are relatively unconservative compared to many situations, and the potential savings from the Pipe Crawler® will often be larger than reported in this analysis.

Three Pipe Crawler® survey instruments are included in developing costs for the innovative technology. The number of pipes and the associated number of pipe crawler sizes will vary with the specific needs of the site. The cost of the equipment is relatively small; consequently, the total cost is not sensitive to the number of pipe crawler sizes required.

Because of the impact that site-specific conditions have on total costs, decision makers should tailor this analysis for their site by substituting the expected quantities, mobilization distance, etc. into Table B-1 of Appendix B.



## SECTION 6

# REGULATORY AND POLICY ISSUES

### Regulatory Considerations

---

The regulatory/permitting issues related to the use of the Pipe Crawler® technology at the ANL CP-5 Research Reactor are governed by the following DOE Orders and safety and health regulations:

#### DOE Orders

- DOE 5400.5 Radiation Protection of the Public and the Environment
- DOE 5480.11 Radiation Protection for Occupational Workers
- DOE 5820.2A Radioactive Waste Management

#### Occupational Safety and Health Administration (OSHA) 29 CFR 1926

- 1926.300 to 1926.307 Tools-Hand and Power
- 1926.400 to 1926.449 Electrical - Definitions
- 1926.28 Personal Protective Equipment
- 1926.52 Occupational Noise Exposure
- 1926.53 Ionizing Radiation
- 1926.55 Gases, Vapors, Fumes, Dusts and Mists
- 1926.102 Eye and Face Protection
- 1926.103 Respiratory Protection

- OSHA 29 CFR 1910

- 1910.211 to 1910.219 Machinery and Machine Guarding
- 1910.241 to 1910.244 Hand and Portable Powered Tools and Other Hand-Held Equip.
- 1910.301 to 1910.399 Electrical - Definitions
- 1910.95 Occupational Noise Exposure
- 1910.132 General Requirements (Personal Protective Equipment)
- 1910.133 Eye and Face Protection
- 1910.134 Respiratory Protection
- 1910.147 The Control of Hazardous Energy (Lockout/Tagout)

In addition to these regulations, the baseline technology would be subject to numerous OSHA regulations covering demolition, excavation, and operation of heavy equipment. The waste form requirements for low-level wastes from either technology, as specified by disposal facilities used by ANL, include:

- *Hanford Site Solid Waste Acceptance Criteria: WHC-EP-0063-4*
- *Barnwell Waste Management Facility Site Disposal Criteria: S20-AD-010*
- *Waste Acceptance Criteria for the Waste Isolation Pilot Plant: WIPP-DOE-069*

Since the Pipe Crawler® technology is designed for the decontamination of structures, there is no regulatory requirement to apply CERCLA's nine evaluation criteria. However, some evaluation criteria required by CERCLA, such as community acceptance, is briefly discussed below. Other criteria, such as cost and effectiveness, were discussed earlier in the document.



## Safety, Risks, Benefits, and Community Reaction

---

The Pipe Crawler® technology is generally quite safe to operate. Identified hazards are those typical of working in industrial situations with electrical powered instrumentation. Physical hazards from working in confined or tight spaces associated with pipe systems are also present. Additionally, a high degree of physical exertion may be needed to maneuver the Pipe Crawler® inside the pipes. Hazards associated with radiological contamination inside piping systems are of potential concern.

Using the Pipe Crawler® technology as a technique to verify the absence of contamination eliminates the unnecessary steps of excavation, dismantlement, and disposal of uncontaminated piping. Risks to workers associated with excavation, heavy equipment usage, and possible exposure to radioactive piping can be eliminated.

The use of the Pipe Crawler® technology rather than the baseline technology would have little impact on community safety, environmental, or socioeconomic issues. Any such impacts would be mostly favorable relative to the baseline technology due to reduced disruption of the affected facility, reduced physical hazards, reduced noise and dust emissions, and reduced waste hauling and disposal.



## SECTION 7

# LESSONS LEARNED

### Implementation Considerations

---

- Pipe Crawler® cannot be used in lines with standing water.
- Pipe surfaces should be fairly smooth and free of debris or sharp edges.
- Pipe Crawler® can be used for initial characterization, but it is best suited for final release surveys after pipe decontamination due to reduced likelihood of cross-contamination.
- Pipes must be free of obstructions or accessible from either side of obstructions.
- Accessibility of pipe systems from both ends gives greater range and improves ability to manipulate crawlers.

Vertical or slick pipes present no problems.

### Technology Limitations and Needs for Future Development

---

- A single crawler can survey only a narrow range of pipe diameters, typically plus or minus .5 in.  
The technology is not well suited to alpha surveys, especially in larger pipes, due to geometry of detectors relative to pipe surfaces.
- Stepwise movement of crawlers is time consuming and labor intensive but yields ample detectability and readily identifies hot spots.
- Units are currently custom made and used as part of a turnkey service, hence current capacity is fairly limited; widespread implementation would probably require considerable "tooling up" of the technology.
- It would be helpful to have software that converted readings from cpm to dpm/100 cm<sup>2</sup> and plotted the results as a profile for each hole or line surveyed for comparison to the 5000 dpm/100 cm<sup>2</sup> release standard.

### Technology Selection Considerations

---

- Pipes should be accessible in intervals of no more than 100 ft from one end or 200 ft from both ends.
- Pipes should be free of loose contamination to prevent the spreading of contamination and false readings.  
Pipe Crawler® is best suited for detection of beta-gamma emitters.
- The feasibility of decontaminating pipes to below release standards should be determined prior to pursuing a management option involving free release based on surveys.



## APPENDIX A

### REFERENCES

- Strategic Alliance for Environmental Restoration, *CP-5 Large-Scale Demonstration Project, Test Plan for the Demonstration of the Pipe Crawler System at CP-5*, November 1996.
- Strategic Alliance for Environmental Restoration, *CP-5 Large-Scale Demonstration Project, Technology Demonstration Summary Sheet, Pipe Crawler Radiological Surveying System*, January 1997.
- Strategic Alliance for Environmental Restoration, *CP-5 Large-Scale Demonstration Project, Summary of Results of Pipe Crawler Surveys from DOE's Large-Scale Demonstration at CP-5*, March 1997
- Occupational Safety and Health Administration, (OSHA) 29 CFR 1910, *Occupational Safety and Health Standards*, 1974.
- Occupational Safety and Health Administration, (OSHA) 29 CFR 1926, *Occupational Safety Regulation for Construction*, 1979.



## TECHNOLOGY COST COMPARISON

This Appendix contains definitions of cost elements, descriptions of assumptions, and computations of unit costs that are used in the cost analysis.

### Innovative Technology: Pipe Crawler®

#### Mobilization

---

##### Transporting Personnel and Equipment

Definition: Transport of vendor's personnel and equipment from New London, Connecticut to site by van, using one crew member as the driver. Although one crew member drove from Texas, the estimate assumes that all crew members travel from New London.

##### Unloading Equipment

Definition: Unloading the vendor's equipment includes time for crew to unpack equipment from the van and move the equipment to a staging area for radiological survey.

Assumptions: 1 h is required for unloading the equipment, based on experience gained during the demonstration.

##### Surveying Equipment

Definition: This cost element provides for radiological survey of the equipment by a site HPT to assure that contaminated equipment is not brought on site. Costs include crew stand-by time plus HPT labor.

Assumptions: 1 h is required for survey, based on experience gained during the demonstration.

##### Training

Definition: Site and Health and Safety-related training is required for subcontractor personnel.

Assumptions: One day is required for training, based on experience gained during the demonstration.

#### Characterization

---

##### Setting Up Each Morning

Definition: This cost element includes time each morning to lay out the equipment and prepare for the day's work.

Assumptions: Set-up is assumed to be 10 min, based upon experience gained during the demonstration.

##### Establishing Background

Definition: The background radiation level is established for each pipe size. Cost will vary depending upon the number of pipe sizes.

Assumptions: Based on vendor's experience, establishing background requires 2 h per pipe size by a health physics technician (HPT). The Pipe Crawler® has eight size increments, with diameters ranging from 2 in–24 in. Jobs will vary in the number of pipe sizes that will be required for establishing background. Additionally, many of the situations requiring characterization will not require a high level of accuracy in determining background. Consequently, the number of background counts that will be required for an individual job will vary from zero (if no background is required) to eight (if all pipe sizes are encountered as part of the work).



## **Accessing Pipe**

Definition: This cost element accounts for the time and equipment required to open a pipe by removing a plug, cap, etc.

Assumptions: During the demonstration of this technology, a crane was used to gain access to the piping in the Rod Storage Area, which had been capped with 500-lb plugs for health and safety reasons. Job sites where this technology may be used will have various plugs, clean-out plugs, drain strainers, valves, or other pipe closures requiring effort to gain access to pipes; therefore, each situation will have a different cost.

## **Videotaping Pipeline**

Definition: Prior to survey, a camera is used to observe the pipe interior.

## **Characterizing Pipe**

Definition: This cost element accounts for the time required to move through the pipeline and characterize it.

Assumption: The time required for movement through the pipeline was very consistent and observed to be 1.2 min per survey measurement. For 10-in and smaller pipes, the measurements were taken at 4-in intervals. For larger pipes, the interval was 12 in.

## **Setting Up and Moving to Adjacent Pipe**

Definition: The time required to clean the cabling and set up on the next pipe (assuming that that pipe is nearby) is estimated in this cost element.

Assumptions: Based on the demonstration, the time required is 10 min to clean the cables and move onto the next pipe.

## **Setting Up and Moving to Remote Pipe**

Definition: This cost element is for moving to pipes that are in other parts of the building or sufficiently remote from the current location that the equipment must be packed for moving.

## **Performance Check**

Definition: This cost element accounts for performing a check of the instrument and system, using a calibrated source to assure that any variation in performance is identified (at the end of the day) and includes the cost of the crew standing by during this time.

Assumptions: The duration of this activity is based on observations during the demonstration and on the vendor's experience. The performance check is assumed to be performed once each day for each pipe size being surveyed. The assumed time for each check is 20 min.

## **HPT Support**

Definition: This cost element consists of one HPT present for the duration of the survey activity.

## **Productivity Loss**

Definition: Losses from productive work occurring during the course of the work can result from personal protective equipment (PPE) changes, ALARA (as low as reasonably achievable), height of reach inefficiencies, etc.

Assumption: A productivity loss factor (PLF) multiplies the work time to account for the necessary activities that do not directly accomplish work (e.g., work breaks) or to account for conditions that result in decreases in production rates (e.g., heat stress). Since the nonproductive activities in the demonstration are atypical of normal D&D work, most of these activities have been screened out of this analysis. In an effort to restore the costs to a more realistic estimate of typical D&D work, a PLF from the baseline is used (from ANL documentation).

## **Health & Safety (H&S)/Project Meetings**

Definition: This cost element provides for safety meeting and project planning meetings during the work.



Assumptions: The estimate assumes one 15-minute safety meeting each day (based on typical practice at ANL).

### PPE Cost Per Day

Definition: This cost element provides for PPE clothing used during the work activity. The following costs are applicable.

Equipment	Quantity in Box	Cost Per Box	Cost Each	No. of Reuses	Cost Each Time Used	No. Used Per Day	Cost Per Day
Respirator			1,933	200	10	1	10.00
Resp. Cartridges			9.25	1	9.25	2	18.50
Booties	200	50.00	0.25	1	0.25	4	1.00
Tyvek	25	85.00	3.4	1	3.4	4	13.60
Gloves (inner)	12	2.00	0.17	1	0.17	8	1.36
Gloves (outer pair)			7.45	10	0.75	1	0.75
Glove (cotton Liner)	100	14.15	0.14	1	0.14	8	1.12
<b>Total</b>							<b>46.33</b>

The PPE costs are predominantly from the ANL activity cost estimates for 1996. (Costs for outer gloves, glove liners, and respirator cartridges are from commercial catalogs.)

Assumption: Four changes each day per person (typical for ANL D&D work).

## Demobilization

### Surveying and Decontaminating

Definition: This cost element provides for radiological survey of the equipment by a site HPT to assure that contaminated equipment does not leave the site and includes costs for decontamination. Costs include crew stand-by time plus HPT labor.

Assumptions: 4 h is required for survey, based on observed time from demonstration.

### Packing Equipment

Definition: Loading the vendor's equipment includes time required for crew to pack equipment in the van.

Assumptions: One h is required for unloading the equipment. This is based on observed times from the demonstration.

### Transporting Personnel and Equipment

Definition: Transporting vendor's personnel and equipment from the site to New London, Connecticut, using one crew member as the driver.

### Labor Cost for Surveying and Decontaminating

Definition: The decontamination and survey of vendor equipment will have some requirement for PPE by the crew and HPT conducting the decon work. This is assumed to be similar to the previously defined PPE cost element.



## Baseline Technology: Dismantlement & Disposal

### Mobilization

#### Transporting and Unloading Equipment

This cost element represents the cost of transporting equipment from a local equipment rental firm to the local site. The costs include loading the equipment on a truck for transport, transporting, unloading, and standing by for equipment being rented. The equipment includes a concrete saw, a backhoe loader, and miscellaneous equipment. Transport costs are shown below.

Crew Element	Unit Rate (\$/h)	Quantity	Total (\$)
<b>Labor</b>			
Truck Driver	49.67	4 h	149.01
<b>Total</b>			149.01
<b>Equipment (rental)</b>			
Concrete Saw (baseline estimate)	17.13	3 h	51.39
Backhoe Loader (baseline est.)	60.78	3 h	182.34
Flat Bed Truck rental (3 ton, Means 1997):	19.00	4 h	76.00
Miscellaneous	5.00	3 h	15.00
<b>Total:</b>			

#### Surveying

Definition: This cost element consists of renting survey equipment and paying labor costs for an HPT to perform the survey.

Assumptions: The survey equipment is dropped off at a staging area. An HPT comes by later to perform the survey. Relevant costs are presented below.

Crew Element	Unit Rate (\$/h)	Quantity	Total (\$)
<b>Labor</b>			
HPT	56.00	1 h	56.00
<b>Total</b>			56.00
<b>Equipment (rental)</b>			
Concrete Saw (baseline estimate)	17.13	4 h	68.52
Backhoe Loader (baseline est.)	60.78	4 h	243.12
Miscellaneous	5.00	4 h	20.00
<b>Total</b>			331.64
<b>Other Costs</b>			
Waste Disposal for Swipes	52.78 \$/ft <sup>3</sup>	1/4 ft <sup>3</sup>	26.39
<b>Total:</b>			26.39

### Dismantlement

#### Concrete Cutting

Definition: This cost element provides for saw cutting the floor, which overlies the piping.

Assumptions: This analysis assumes the floor is cut using a diamond saw, which makes two parallel cuts that are approximately 1 ft to 18 in apart and then cross cuts are made at intervals of approximately 18 in.



The production rate of 2 ft/h per linear ft of trench length is based on rates from the 1992 baseline (ANL, 1992).

### Removing Concrete Block

Definition: This cost element provides for the removal of the block of concrete that is cut from the floor.

Assumptions: The block is assumed to be removed using a backhoe loader. The equipment and production rate of 4 ft/h is based on the 1992 baseline (ANL, 1992).

### Removing Pipe and Contaminated Soil

Definition: Once the concrete has been removed, then the piping and any contaminated soil is removed.

Assumption: The production rate is 7 ft/h, based on the 1992 baseline (ANL, 1992).

### HPT Support

This cost element is the same as the cost element for Pipe Crawler®.

### Productivity Loss

Definition: Losses for donning and doffing, etc. are accounted for in this cost element.

Assumption: Productivity loss (associated with changing of PPE, etc.) is assumed to be the same as used in the baseline estimate (ANL, 1992) and is 1.10 for concrete removal activities and 2.02 for pipe removal activities.

### H&S/Project Meetings

This cost element is similar to the cost element for the Pipe Crawler®.

### PPE Cost Per Day

Applicable costs are presented below.

Equipment	Quantity in Box	Cost Per Box	Cost Each	No. of Reuses	Cost Each Time Used	No. Used Per Day	Cost Per Day
Respirator			1,933	200	10	1	10.00
Resp. Cartridges			9.25	1	9.25	2	18.50
Booties	200	50.00	0.25	1	0.25	4	1.00
Tyvek	25	85.00	3.4	1	3.4	4	13.60
Gloves (inner)	12	2.00	0.17	1	0.17	8	1.36
Gloves (outer pair)			7.45	10	0.75	1	0.75
Glove (cotton Liner)	100	14.15	0.14	1	0.14	8	1.12
<b>Total</b>							<b>46.33</b>

PPE costs are predominantly from the ANL activity cost estimates for 1996. (Costs for outer gloves, glove liners, and respirator cartridges are from commercial catalogs.)

Assumption: D&D work at ANL typically requires four changes each day per person.



## Demobilization

---

### Decontaminating and Surveying

Definition: This cost element consists of renting survey equipment and the paying the labor cost for an HPT to perform the survey. Applicable costs are presented below.

Crew Element	Unit Rate (\$/h)	Quantity	Total (\$)
Labor			
HPT	56.00	8 h	448.00
<b>Total</b>			<b>448.00</b>
Equipment (rental)			
Concrete Saw (baseline estimate)	17.13	8 h	137.04
Backhoe Loader (baseline est.)	60.78	8 h	486.24
Miscellaneous	5.00	8 h	40.00
<b>Total</b>			<b>663.28</b>
Other Costs			
LL Waste Disposal	52.78 \$/ft <sup>3</sup>	1	52.78
<b>Total:</b>			<b>52.78</b>

### Productivity Loss

Definition: Decontamination and survey of rented equipment will have some productivity loss. This analysis assumes an amount of loss consistent with the 1992 baseline (ANL, 1992) of 1.10.

### PPE Cost

Definition: Decontamination and survey of rented equipment will have some requirement for PPE by the HPT conducting the decon work. This is assumed to be similar to the previously defined PPE cost element.

## Waste Disposal

---

### Clean Waste (Concrete)

Definition: This cost element provides for disposal of the concrete blocks cut from the floor.

Assumption: The blocks are assumed to be free of contamination (a common assumption for this type of work) so that they can be disposed of as clean waste. Rate of \$0.14/ft<sup>3</sup> for packaging, transport, and disposal are from ANL 1996 activity cost estimates. The 1992 baseline documentation (ANL, 1992) does not provide for any swell of the concrete waste (assumes that blocks are neatly stacked).

### Waste Disposal (Solid, Low-Level Radioactive Waste)

Definition: This cost element provides for the disposal of contaminated soil and pipe.

Assumption: The contamination is assumed to be low-level radioactive waste, and the disposal cost is \$53/ft<sup>3</sup> based on rates from ANL 1996 activity cost estimates. The 1992 baseline documentation (ANL, 1992) assumes a 150 percent swell factor and 0.05 ft<sup>3</sup>/ft of contaminated soil.



### Innovative Technology: The Pipe Crawler®

Costs for demonstrating the Pipe Crawler® innovative technology are based on operating the device at two encased pipe locations—the rod storage area, and area containing air lines connecting to the reactor area. The Pipe Crawler® technology consists of mobilization, site-specific training, set-up, establishing background counts, removing any caps or obstructions to the pipeline entrance, videotaping the pipeline interior, radiological survey of the pipeline interior, moving and setting up on the next pipe, conducting performance checks, and demobilization. The projection of demonstration costs to reflect a more realistic cost for that scope of work include a number of assumptions that make that projection possible. These assumptions are shown below:

- Survey of pipe consists of one pass through the pipe. Time requirements associated with multiple passes through the pipe to check survey repeatability are ignored since this should not be necessary for typical D&D work situations.

Those surveys where alternative instrument movement distances are used are not considered in this analysis; only those surveys covering approximately 25 percent of the pipe interior surface are used because the Nuclear Regulatory Commission (NRC) has previously accepted the 25 percent coverage rate.

Surveys of pipes using less than 1-min count times are not included since this is not the currently accepted standard. Alternate count times were performed to facilitate comparison with the standard 1-min count.

Surveys having variations in normal procedures (such as not being able to rotate the detector to the off-set position) are not included since this does not conform to standard practice.

Seven hours of meetings (associated with planning the demonstration, debriefing for an alpha contamination incident, and data collection questioning) are excluded. Included are the morning safety meetings (15 min per day of work).

The time required to convert a 6-in-diameter Pipe Crawler® to fit a 5-in-diameter pipe is omitted from this analysis. Normal work practice is better represented by including the equipment cost for a 5-in, 6-in, and 12-in-diameter Pipe Crawler® rather than show the cost for two pipe crawlers and time required to convert from one size to the other.

Work will be performed as a vendor-provided service, rather than purchase the equipment and perform work with local craft because the following operation issues made ownership prohibitive:

- The number of Pipe Crawler® survey instruments required to cover the potential range in pipe sizes is large.
- The expense of the calibration standards is high.
- Unique skill is required for some of the periodic maintenance of the equipment.

Equipment hourly rates were based upon the depreciated purchase price and maintenance cost of the equipment reported by the vendor. The labor rates are based on rates provided by the vendor. Depreciation is based on a cost of money at 6.375 percent, determined by the Secretary of the Treasury pursuant to Public Law 92-41, 85 Statute 97 and discounted to 4.78 percent, service life of three–five years (depending on the individual piece of equipment), straight-line depreciation, repair cost for periodic maintenance, and assumed use of 800 h/yr.

Full-time HPT support is included.

A productivity loss factor (PLF) multiplies the work time to account for the necessary activities that do not directly accomplish work (e.g., work breaks) or to account for conditions that result in decreases in production rates (e.g., heat stress). Since the nonproductive activities in the demonstration are atypical of normal D&D work, most of these activities have been screened out of this analysis. In an effort to restore the costs to a more realistic estimate of typical D&D work, a PLF from the baseline is used (from ANL documentation of budgets developed in 1992) and is 1.10 based on the factors as shown.



Base	1.00
+Height	0
+Radiological/ALARA	0
+Protective Clothing	0
<hr/>	
= Subtotal	1.00
X	
Respiratory Protection	1.00
<hr/>	
=Subtotal	1.00
X	
Breaks	1.10
<hr/>	
=Total	1.10

- Procurement cost of 9.3 percent is added to the hourly rate for the vendor-owned equipment and the vendor labor to account for the ANL charge to the project for administration of the procurement contract.

The cost for PPE used during the demonstration is based upon typical practice and equipment at ANL (four pairs of PPE used each day per person). Since this is an assumed rate rather than an observed quantity, the cost is computed based on the total duration of work in the controlled area plus the time required for decontamination of the equipment at the completion of the work.

During the course of the demonstration, it was observed that the duration and effort required for the radiological survey was consistent for all pipes for the duration of the demonstration. Costs for mobilization and demobilization will vary from site to site depending upon the mobilization distance.

The activities, quantities, production rates, and costs observed during the demonstration are shown in Table B-1, Innovative Technology Cost Summary.



Table B- innovative technology Cost Summary

Work Breakdown Structure (WBS)	Unit Cost (UC)			Total UC	Total Quantity (TQ)	Unit of Measure	Total Cost (TC) note	Comments	
	Labor H Rate	Equipment H Rate	Other						
<b>MOBILIZATION (WBS 331.01)</b>									
Transport Personnel & Equip	10	\$ 195	10	\$ 78	\$ 2,731	2 Day	\$ 8,261	New London, CT. to Chicago (Department of Transportation (DOT) restrictions approx. 500 miles per day & 10 h/day) crew of 2 vendor personnel (consistent for remainder of table)	
Unload Equipment (Equip)	1	\$ 195	1	\$ 78	\$ 273	1 Each	\$ 273		
Survey-In Equip	1	\$ 195	1	\$ 78	\$ 273	1 Each	\$ 342		
Vendor Crew Stand-By HPT Support	1	\$ 56	-	-	\$ 69			Vendor Labor & Equipment rates ANL's Health Physics Technician (HPT) labor and 1/4 ft <sup>3</sup> of Low Level waste disposal for swipes @ \$52.78/ft <sup>3</sup>	
Worker Training	8	\$ 195	8	\$ 78	\$ 2,185	1 Day	\$ 2,185	Site training plus Rad Worker II Training	
<b>PIPE CHARACTERIZATION (WBS 331.17)</b>									
Set-Up Each Morning	0.167	\$ 195	0.167	\$ 78	\$ 46	3 Day	\$ 137	10 min of set-up per day of work	
Establish Background					\$ -		\$ -	Assume 2 h/ pipe size for HPT to establish background (not performed for this demo)	
Access Pipeline	0.083	\$ 195	0.083	\$ 78	\$ 23	15 Pipes	\$ 441	Lift 500 pound cap off rod storage pipe	
Vendor Stand-By	0.083	\$ 40	0.083	\$ 40	\$ 7			ANL crane operator and overhead crane	
Lift Cap off Pipe	0.012	\$ 195	0.012	\$ 78	\$ 3	212 Ft	\$ 683		
Video Pipeline	0.059	\$ 195	0.059	\$ 78	\$ 16	49 Ft	\$ 792		
Pipe Survey - 10 in & Smaller	0.02	\$ 195	0.02	\$ 78	\$ 5	116 Ft	\$ 628	1.2 min for counting + advancement per 4 in	
Pipe Survey - Larger than 10 in	0.004	\$ 195	0.004	\$ 78	\$ 1	709 Pipes	\$ 765	1.2 min. for counting + advancement per 12 in	
Set-Up & Move to Adjacent	1.25	\$ 195	1.25	\$ 78	\$ 341	1 Each	\$ 341	10 min to remove cables and move	
Set-Up & Move to Remote	0.084	\$ 195	0.084	\$ 78	\$ 23	5 Each	\$ 115	Move from inside building to outside	
Performance Check	15.17	\$ 56			\$ 850	1 Each	\$ 850	5 min per check per day per pipe size	
HPT Support	3.03	\$ 195	3.03	\$ 78	\$ 827	1 Each	\$ 827	HPT presence during performance of work (PLF=1.10)	
Productivity Loss Factor(PFP)	0.25	\$ 195	0.25	\$ 78	\$ 68		\$ 137	Duration in controlled area X 10 percent	
H&S/Project Meetings					\$ 46	2	\$ 278	15 min/day safety meeting (typical for ANL)	
PPE					\$ -	6	\$ 46	Assumed cost per person per day of \$46.33	
<b>DEMOBILIZATION (WBS 331.21)</b>									
Survey Equip. & Decon	1	\$ 195	1	\$ 78	\$ 273	1 Each	\$ 342	Vendor Labor & Equipment rates	
Vendor Crew Stand-By	1	\$ 56			\$ 69			Same as Mobilization, HPT Support	
HPT Support	1	\$ 195	1	\$ 78	\$ 273	1 Each	\$ 273		
Pack Equipment	10	\$ 195	10	\$ 78	\$ 2,731	2 Day	\$ 5,461	Same as Mobilization, Personal & Equip Trans;	
Personnel & Equip. Transp.	0.1	\$ 195	0.1	\$ 78	\$ 27	1 Each	\$ 27	Applied to decontamination & Survey of Equip	
Productivity Loss Factor					\$ -				
<b>TOTAL:</b>								<b>\$20,358</b>	

Note: TC = UC \* TQ



## Baseline Technology: Dismantle and Disposal

The work is assumed to consist of mobilization of the rented equipment, removal of overlying concrete, removal of piping, survey of concrete to allow disposal as clean waste, packaging of waste, demobilization of equipment, and disposal of waste. The costs for the dismantlement and disposal alternative are based upon production rate and crew cost assumptions developed from historic experience and assumes that the pipe to be removed lies below a concrete floor. The baseline assumed for this analysis does not necessarily reflect the cost or nature of the work that is required to D&D the pipes surveyed by Pipe Crawler<sup>®</sup> during the demonstration. Rather, the baseline reflects a typical approach to D&D work for the types of pipes that are candidates for the Pipe Crawler<sup>®</sup> technology. The assumptions for the baseline are shown below:

- Work is performed using rented equipment and local crafts.
- Concrete is removed to a depth of 1 ft and a width of 18 in.
- Production rates are as follows:
  - 2 ft<sup>3</sup>/h for concrete saw cut
  - 4 ft<sup>3</sup>/h for concrete block removal
  - 7 ft<sup>3</sup>/h for pipe removal
- Pipe waste volume is 150 percent of the actual pipe volume due to bulking. Contaminated soil volume is 0.05 ft<sup>3</sup>/ft (ANL, 1992).
- Concrete waste volume is not adjusted for bulking (assumes concrete blocks are stacked to preclude voids) (ANL, 1992).
- Soil is not contaminated.

Productivity loss (associated with changing of PPE, etc.) is assumed to be the same as used in the baseline estimate (ANL, 1992) and is 1.10 for concrete removal activities and 2.02 for pipe removal activities.

- Safety meetings each morning for 15 min.
- HPT support is full time and provides for safety oversight as well as radiological surveys for segregation of the concrete, soil, and pipe waste.

The costs for dismantlement and disposal will vary from the costs and assumptions used in this analysis due to site-specific conditions. Conditions that will influence cost significantly are depth of concrete overlying the pipe, type of pipe, and disposal costs.

The activities, quantities, production rates, and costs observed during the demonstration are shown in Table B-2, Baseline Technology Cost Summary.



Table B-2. Base Line Technology Cost Summary

Work Breakdown Structure (WBS)	Unit Cost (UC)				Total Quantity (TQ)	Unit of Measure	Total Cost (TC) note	Comments
	Labor H Rate	Equipment H Rate	Other	Total UC				
<b>Mobilization (WBS 331.01)</b>					<b>Subtotal</b>	<b>\$ 1,720</b>		
Transport and Unload Equip.	0 \$	0 \$	\$ 325	\$ 325	1 Each	\$ 325	Transport equipment (Equip.) from local rental, includes 4 h truck hauling, teamster and stand by for saw and backhoe for 3 h	
Survey-in Equipment Stand By HPT Support	0 \$ 1 \$ 56.00	4 \$ 331.64	\$ 13	\$ 1,327 \$ 69	1 Each	\$ 1,396	Stand by cost for saw and backhoe for 4 h ANL's Health Physics Technician (HPT) labor & 1/4 ft <sup>3</sup> of low level (LL) waste disposal for swipes @ \$52.78/ft <sup>3</sup>	
<b>Dismantlement (WBS 331.17)</b>					<b>Subtotal</b>	<b>\$ 41,296</b>		
Concrete Cutting	0.5 \$ 73.45	0.5 \$ 82.91		\$ 78	165 Ft	\$ 12,900	2 ft/h production rate	
Concrete Block Removal	0.25 \$ 73.45	0.25 \$ 82.91		\$ 39	165 Ft	\$ 6,450	4 ft/h production rate	
Remove Pipe & Soil	0.143 \$ 73.45	0.143 \$ 82.91		\$ 22	165 Ft	\$ 3,689	7 ft/h production rate	
Set-Up & Move Remote HPT Support	1 \$ 73.45 148.3 \$ 56.00	1 \$ 82.91		\$ 156 \$ 8,307	1 Each 1 Each	\$ 156 \$ 8,307	HPT presence during performance of work	
Productivity Loss (Concrete)	12.38 \$ 73.45	12.38 \$ 82.91		\$ 1,935	1 Each	\$ 1,935	Work duration in controlled area X 10 percent Productivity Loss Factor (PLF)=1.10	
Productivity Loss (Pipe)	24.07 \$ 73.45	24.07 \$ 82.91		\$ 3,763	1 Each	\$ 3,763	Duration in controlled area X 1.02 percent (PLF=2.02)	
H&S/Project Meetings	0.25 \$ 73.45	0.25 \$ 82.91		\$ 39	23 Days	\$ 899	15 min/day health and safety (H&S) meeting (typical ANL)	
Personal Protection Equip.	0 \$	0 \$	\$ 139	\$ 139	23 Days	\$ 3,197	\$46.33/person/day for 3 persons for 23 days	
<b>Demobilization (WBS 331.21)</b>					<b>Subtotal</b>	<b>\$ 1,546</b>		
Decon and Survey Equip. Equipment Stand By HPT Support	0 \$ 8 \$ 56.00	8 \$ 82.91	\$ 53	\$ 663 \$ 501	1 Each	\$ 1,164	Stand by during decontamination (decon.) ANL's HPT labor rate & 1 ft <sup>3</sup> of Low Level waste disposal for cleaning @ \$52.78/ft <sup>3</sup>	
Productivity Loss Factor	0.08 \$ 56.00	0.08 \$ 82.91		\$ 11	1 Each	\$ 11	Productivity Loss Factor of 1.10 for decon	
Personal Protection Equip.	0 \$	0 \$	\$ 46	\$ 46	1 Day	\$ 46	\$46.33/person/day for 1 persons for 1 day	
Load and Transport Equip.	0 \$	0 \$	\$ 325	\$ 325	1 Each	\$ 325	Same as Mobilization, Transport & Load Equip.	
<b>Waste Disposal (WBS 331.18)</b>					<b>Subtotal</b>	<b>\$ 3,729</b>		
Clean Waste (Concrete)			\$ 0.14	\$ 0.14	248 Cubic Ft	\$ 35	\$0.14/ft <sup>3</sup> unit rate for ANL clean waste disposal	
Waste Disposal (Solid LL)			\$52.78	\$ 52.78	70 Cubic Ft	\$ 3,695	Assume 150 percent bulking for 6 in pipe and 0.05 cubic ft/ft <sup>3</sup> contaminated soil at \$52.78/ft <sup>3</sup> unit rate for ANL LL waste disposal	
<b>TOTAL</b>						<b>\$48,292</b>		

Note: TC = UC \* TQ



## APPENDIX C

### ACRONYMS AND ABBREVIATIONS

ALARA	as low as reasonably achievable
ANL-E	Argonne National Laboratory-East
cm	centimeter(s)
cpm	counts per minute
CP-5	Chicago Pile-5
D&D	decontamination and decommissioning
DDFA	Deactivation and Decommissioning Focus Area
Decon.	Decontamination
DOE	U.S. Department of Energy
DOT	U.S. Department of Transportation
dpm	disintegrations per minute
Equip.	Equipment
ESH	Environment, Safety, and Health
FCCM	facility's capital cost of money
ft	foot (feet)
GM	Geiger Mueller
h	hour(s)
H&S	Health and Safety
HP	health physics
HPT	health physics technician
IH	industrial hygiene
in	inch(es)
lin ft	linear foot (feet)
LSDP	Large-Scale Demonstration Project
min	minute(s)
NRC	Nuclear Regulatory Commission
OSHA	Occupational Safety and Health Administration
PLF	productivity loss factor
PPE	personnel protective equipment
Radial Services, Inc.	RCI
RSH	rod storage holes
TQ	total quantity
UC	unit cost
USACE	U.S. Army Corps of Engineers
WBS	Work Breakdown Structure
WMO	waste management operations
yr	year(s)

